

FIG. 2

Patient  
Push Button

36

34 External  
Stimulator  
Electronics  
(Direct  
electrical  
stimulation  
mode)

40

2

42

4

32

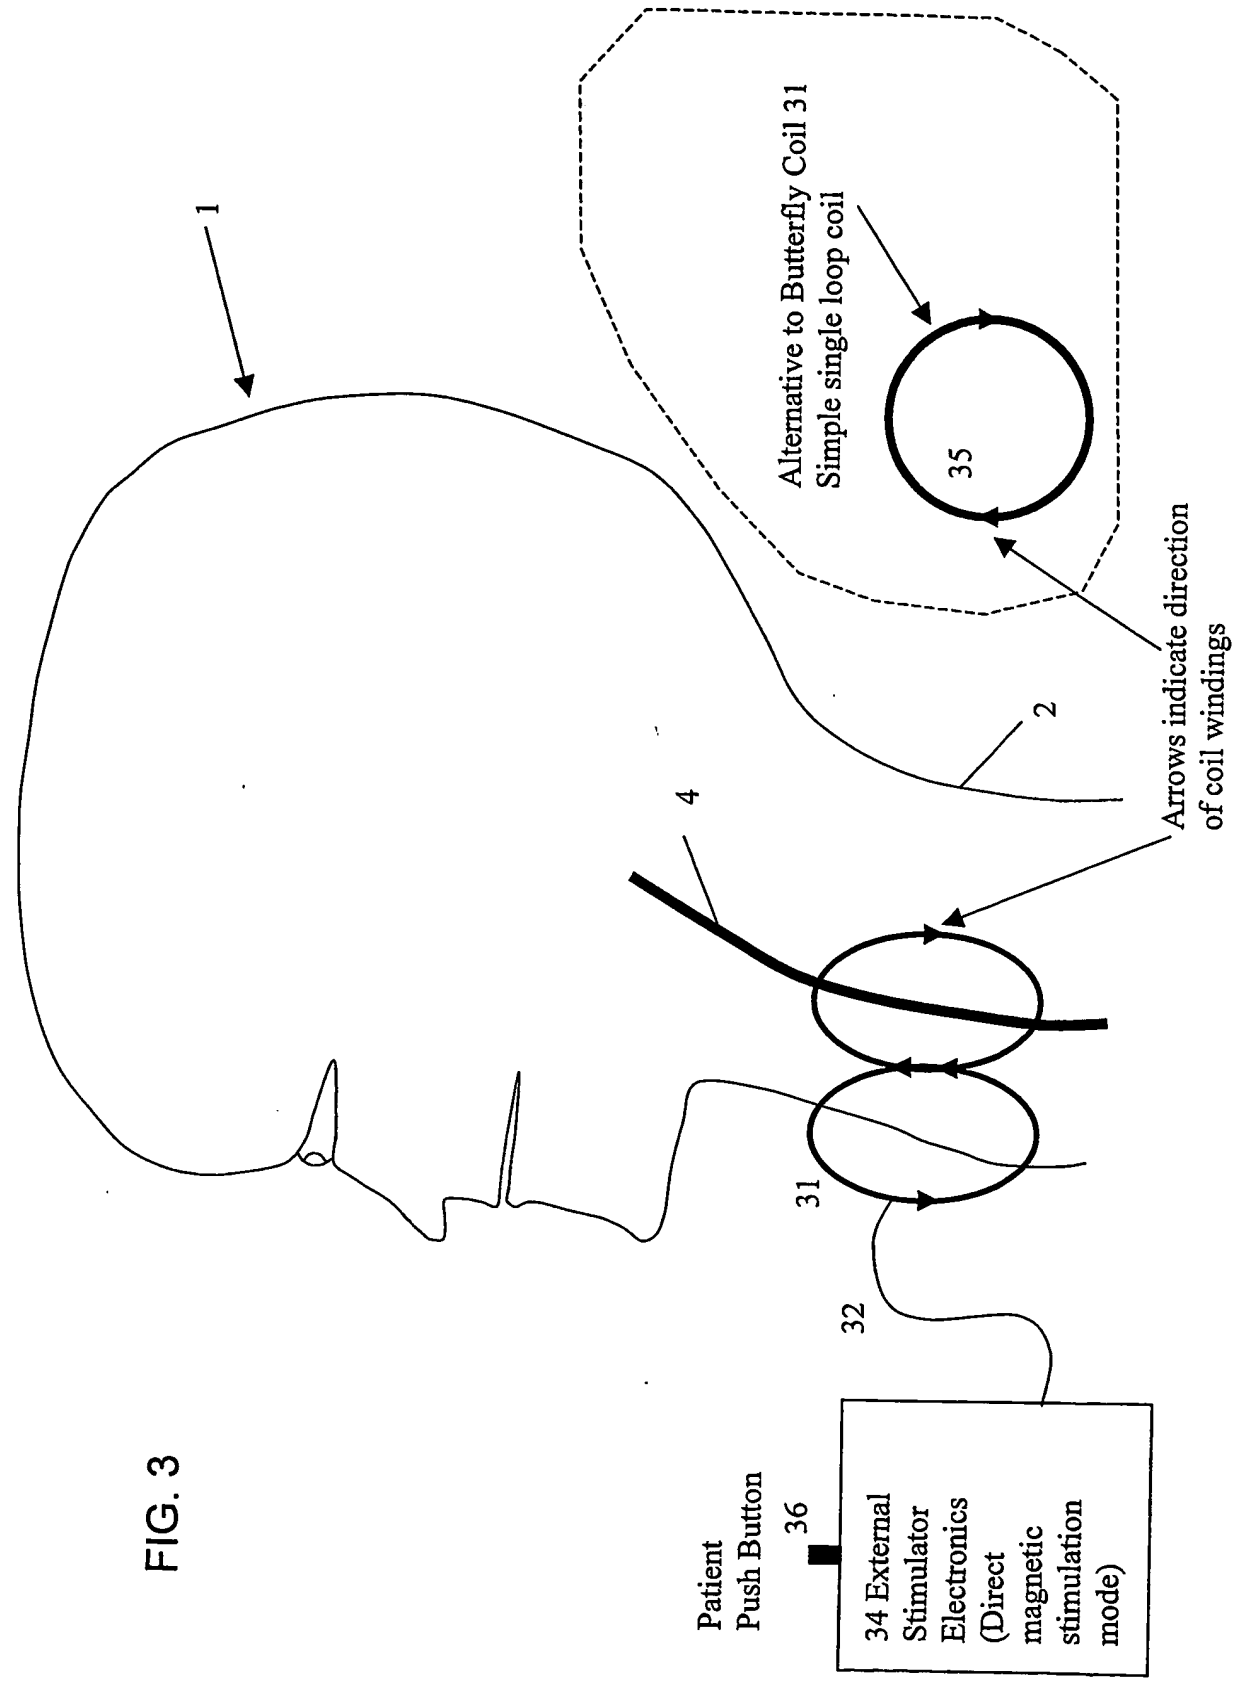


FIG. 4B

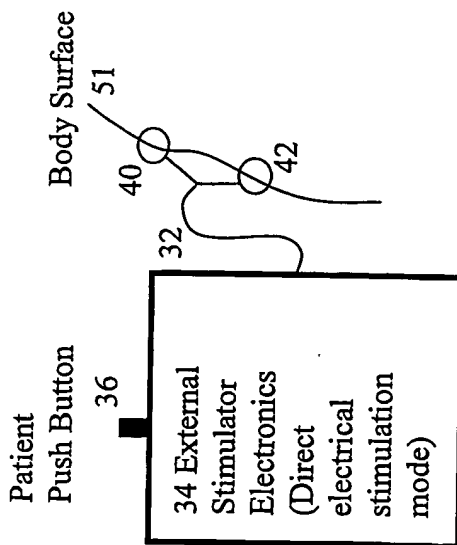


FIG. 4A

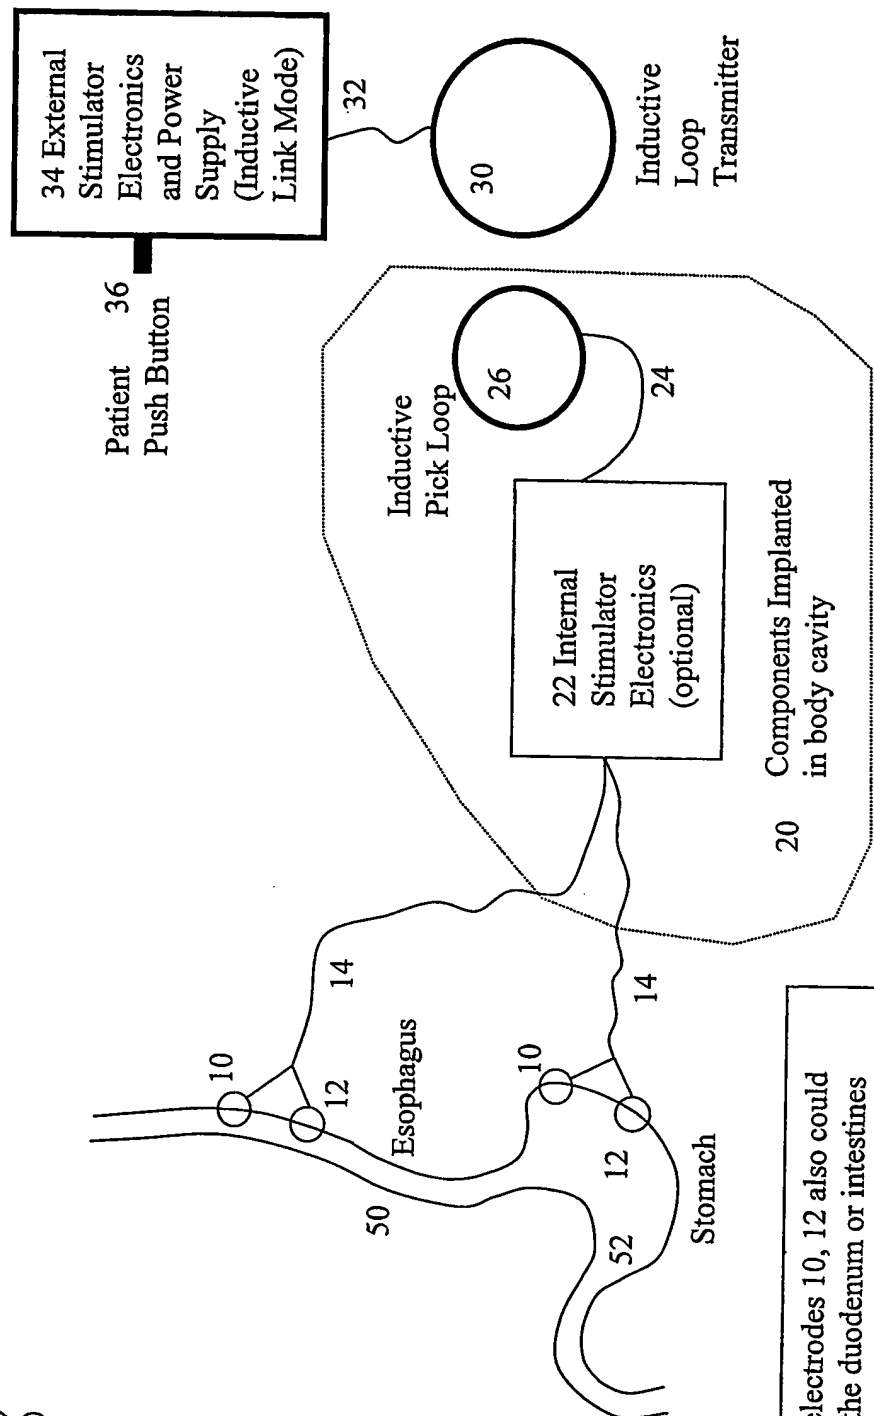


FIG. 5B

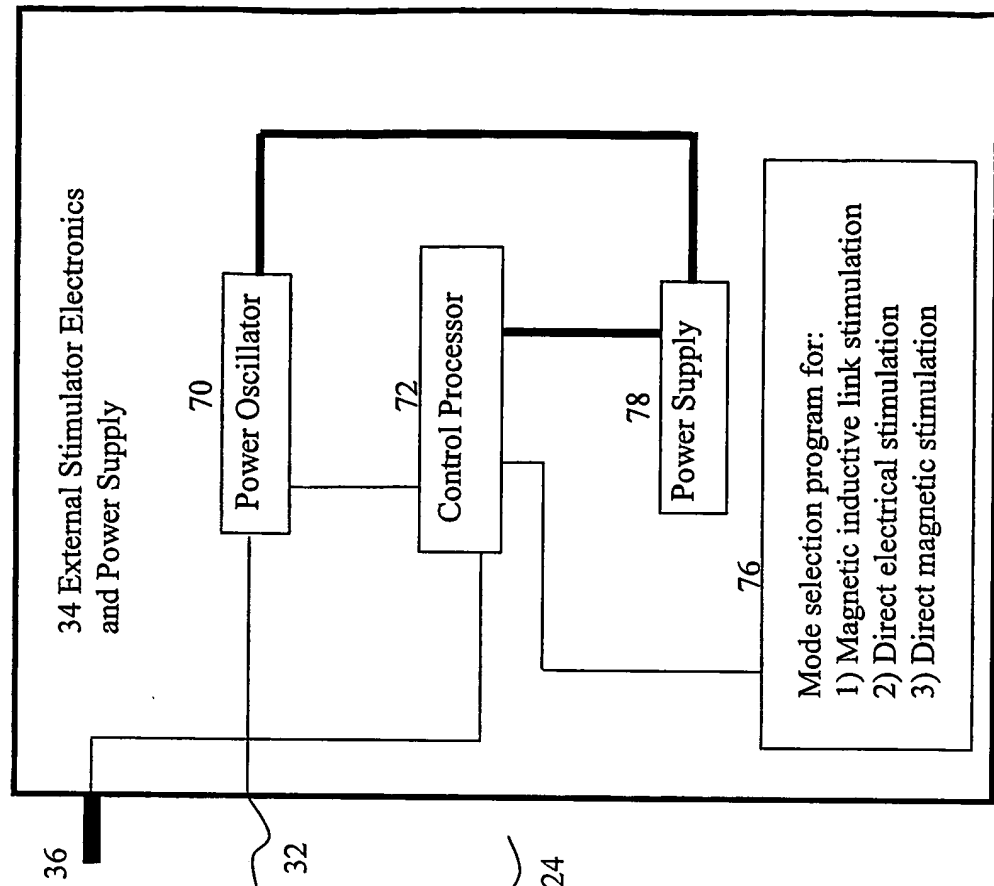


FIG. 5A

